



Pasteur Lille 16 color 100u-20PSI GFP

Cytometer:	FACSriaII	User:	Administrator
Cytometer Name:	FACSriaII	Institution:	N/A
Serial Number:	1	Software:	BD FACSDiva 8.0.1
Input Device:	Manual	Date:	1/26/2018 10:30:03 AM
Sheath Pressure:	20.00		
Nozzle Size:	100		
Window Extension:	2.00		


Red Laser (633nm)

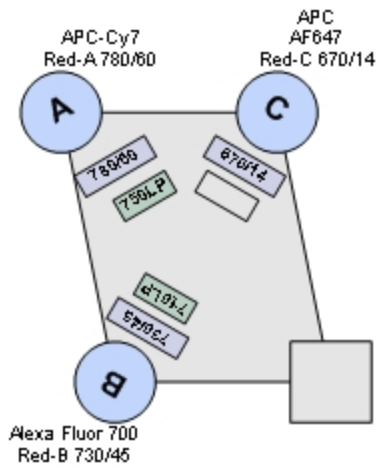


Blue Laser (488nm) FSC

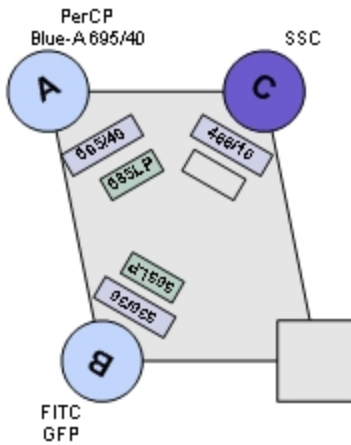

Violet Laser
(405nm)

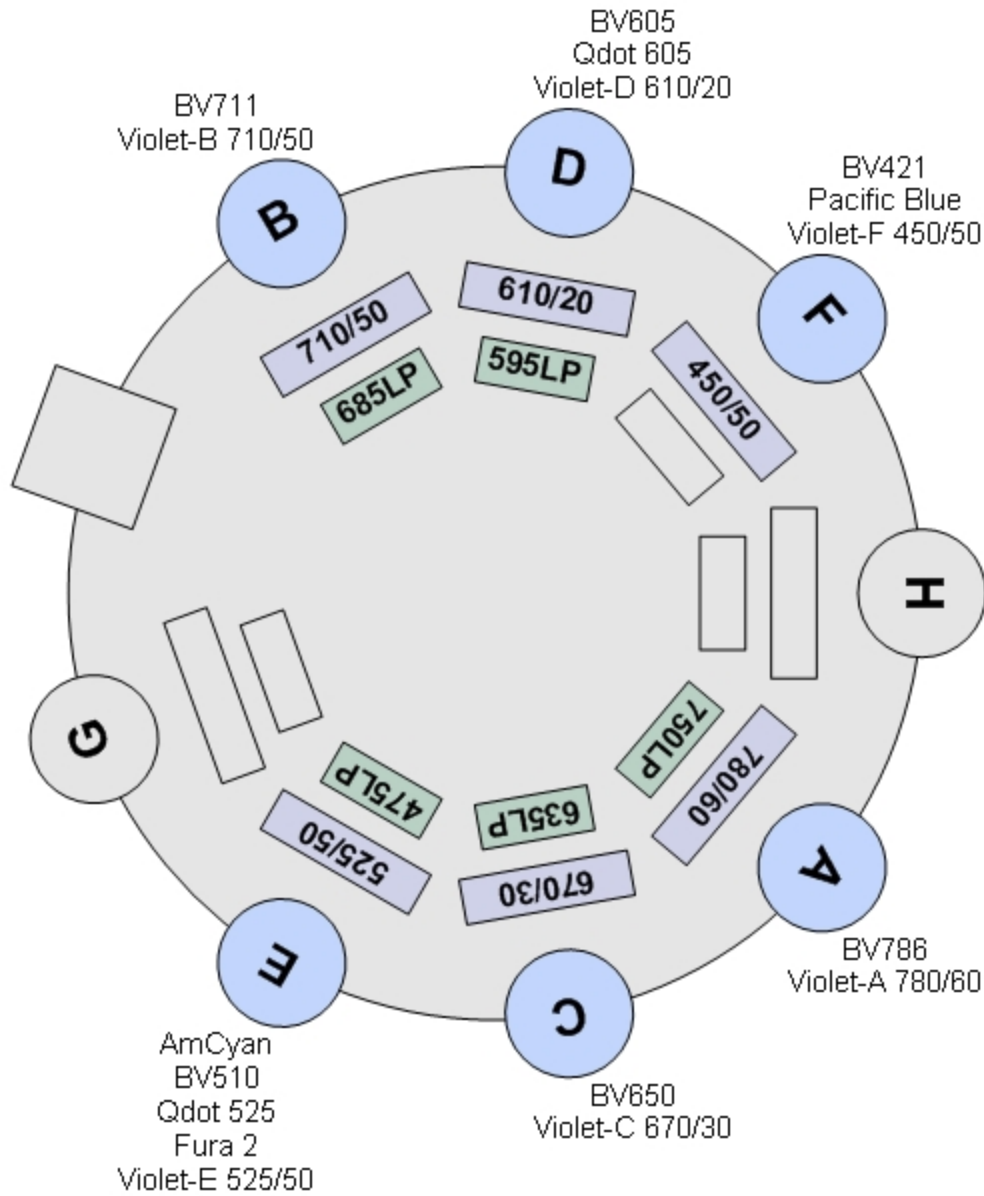

561 Yellow-green Laser
(561nm)

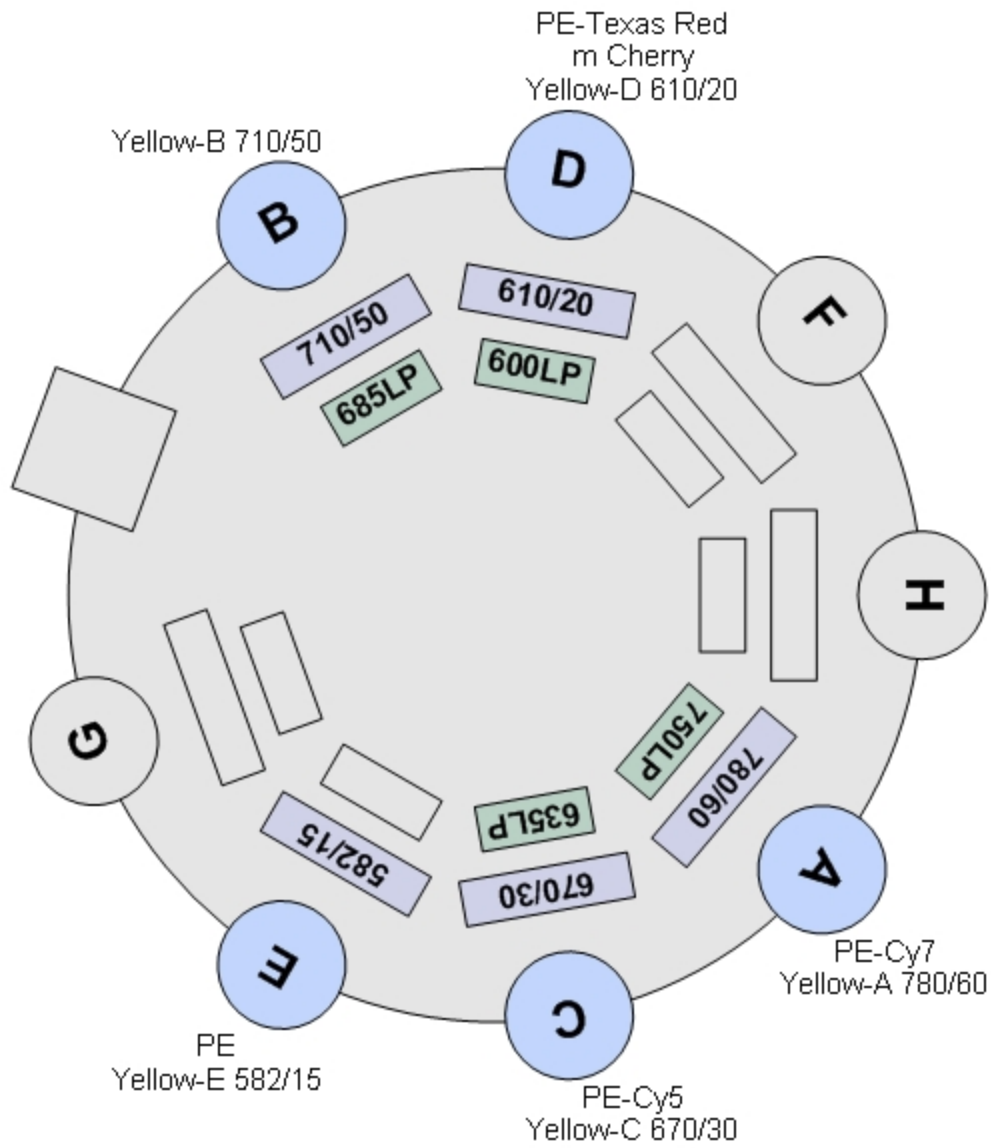

Comments: